



Conventional Setup of Force FX™ Electrosurgical Generator

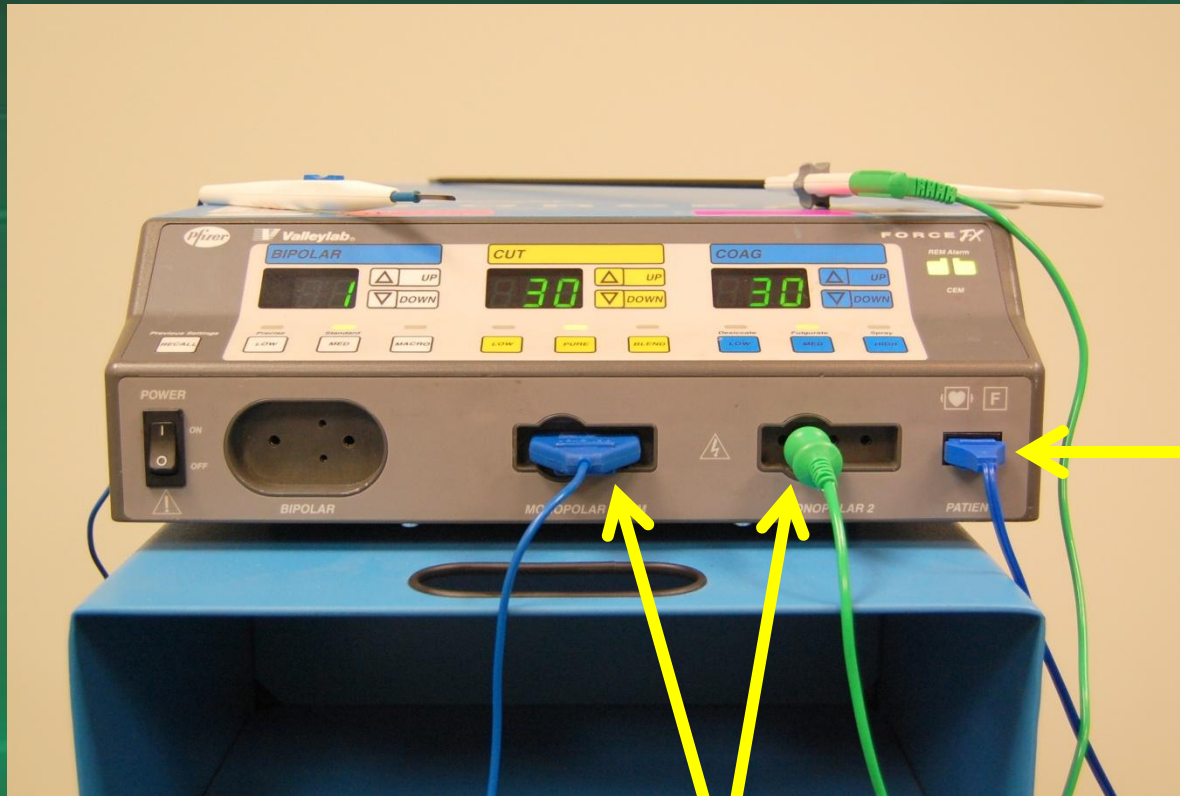

Patient
Return
Electrode
Receptacle

Monopolar Instrument Receptacle

Setup of Force FX™ Electrosurgical Generator with AEM® Monitor and AEM Laparoscopic Instruments

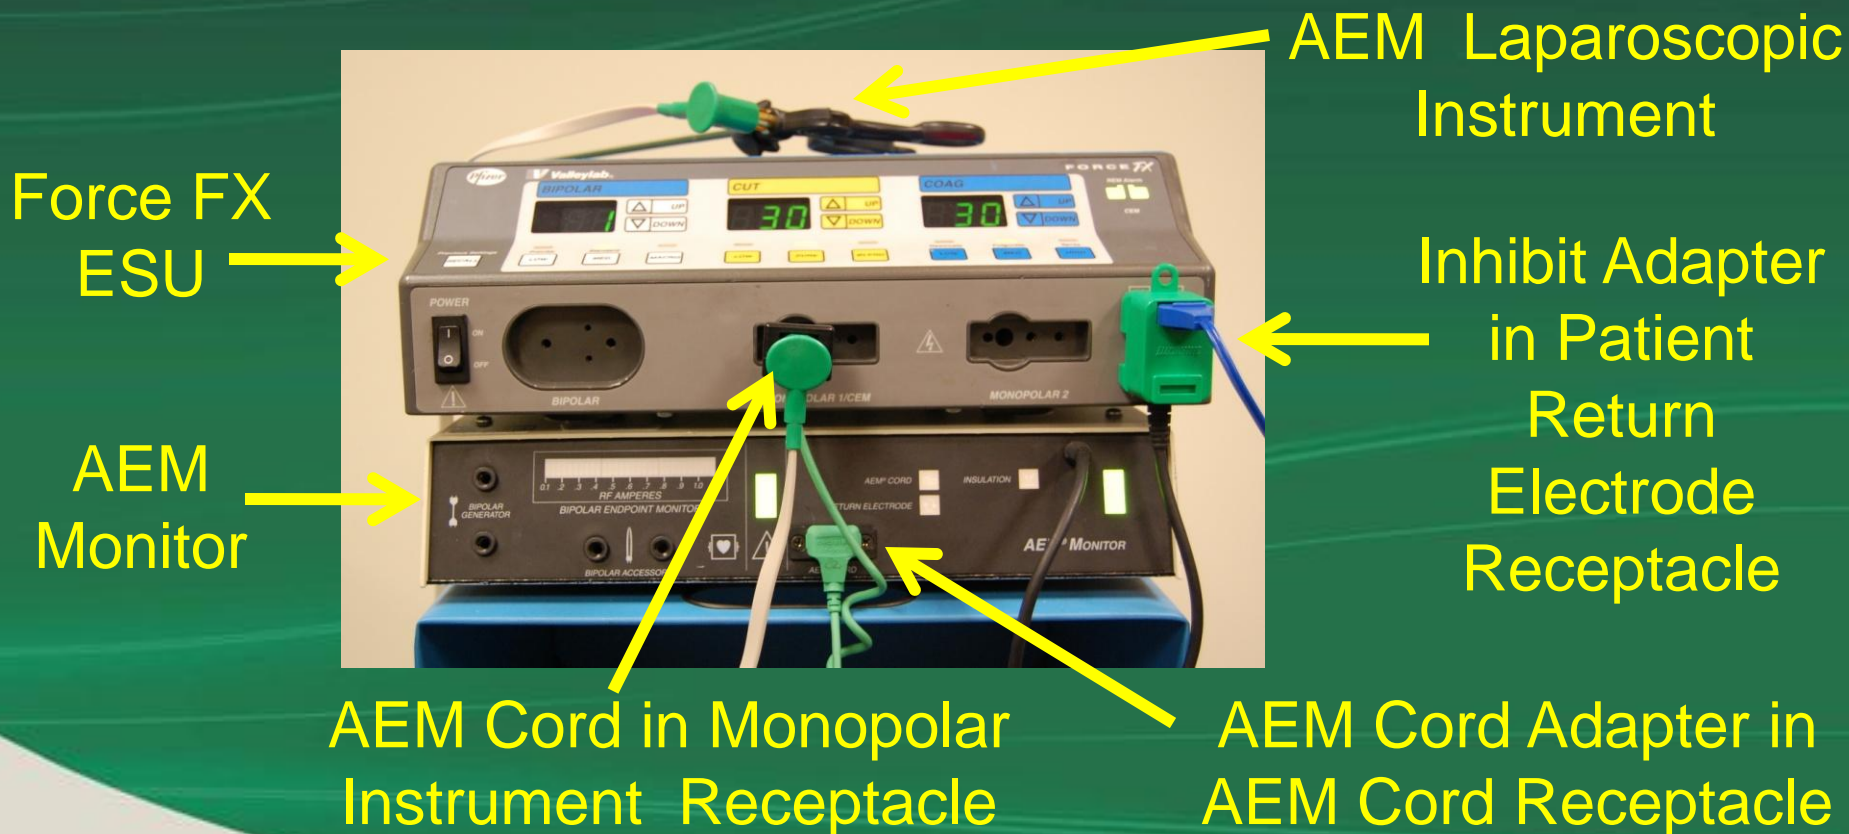

Setup of Force FX™ Electrosurgical Generator with AEM® Monitor and AEM Laparoscopic Instruments

